

Adeno Respi-Strip


Rapid diagnostic test for *in vitro* detection of Respiratory Adenovirus in nasopharyngeal secretions and/or culture supernatants

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')



www.corisbio.com

Adeno Respi-Strip

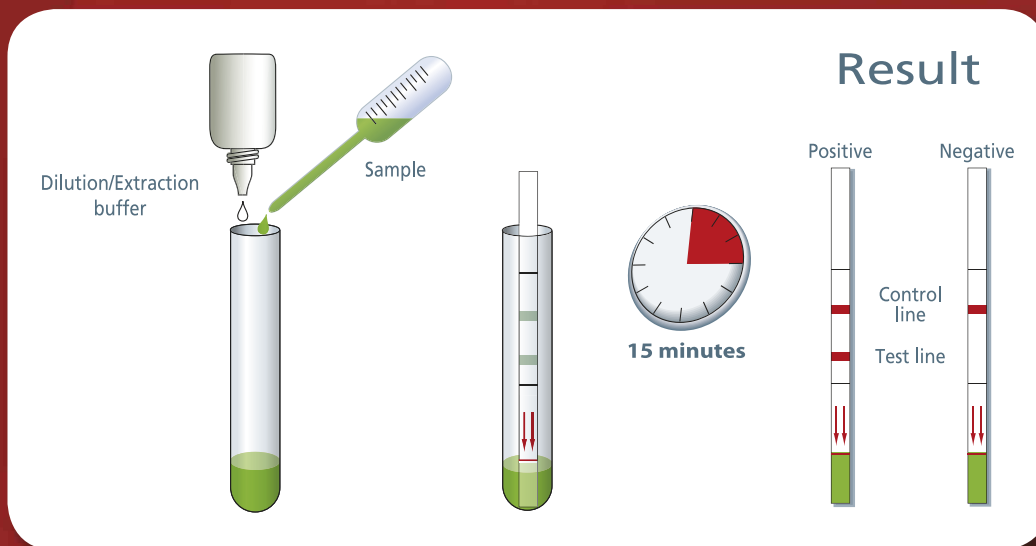

Performance compared to

	ICT competitor 1 (n=127)	ICT competitor 2 (n=127)
Specificity	94.8% (73/77)	96% (72/75)
Sensitivity	94% (47/50)	92.3% (48/52)
PPV	92.15% (47/51)	94.1% (48/51)
NPV	92.1% (73/76)	94.7% (72/76)
Accuracy	94.5% (120/127)	94.5% (120/127)

For more technical information

client.care@corisbio.com


Ordering Information

Product Name	Description	Storage	Code
Adeno Respi-Strip	25 tests, buffer	4°C to 30°C	C-1009
Adeno Respi K-SeT	20 cassettes, buffer	4°C to 30°C	K-1209
Adeno Respi K-SeT, with collection set	20 cassettes, buffer, 20 swabs	4°C to 30°C	K-1509

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus, Mefloquine, Proguanil, *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

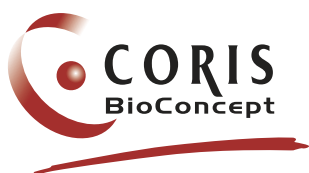

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

Fo 7.5-32-09/06
January 2012